

Selection guide

Amersham ECL Western blotting detection reagents



Choose the ECL Western blotting detection reagent that best suits your needs

Enhanced chemiluminescent (ECL™) detection is based on antibodies conjugated to horseradish peroxidase (HRP). HRP catalyzes the oxidation of luminol in the presence of peroxide, generating emission of low intensity light at 428 nm. The signal intensity is dependent of the number of HRP molecules, and accordingly proportional to the amount of antibody bound to the target molecule (Fig 1).

Since the early 1990s, Cytiva has continuously developed enhanced chemiluminescence detection systems, which today are among the most widely used detection reagents for Western blotting applications. Cytiva offers a variety of chemiluminescence detection reagents, with the best choice depending on the aim of the experiment.

- 1 Detection reagent reacts with HRP and generates light emission
- 2 HRP-conjugated secondary antibody recognizes the primary antibody
- 3 Primary antibody binds specifically to the target protein
- 4 Proteins on membrane after transfer from gel

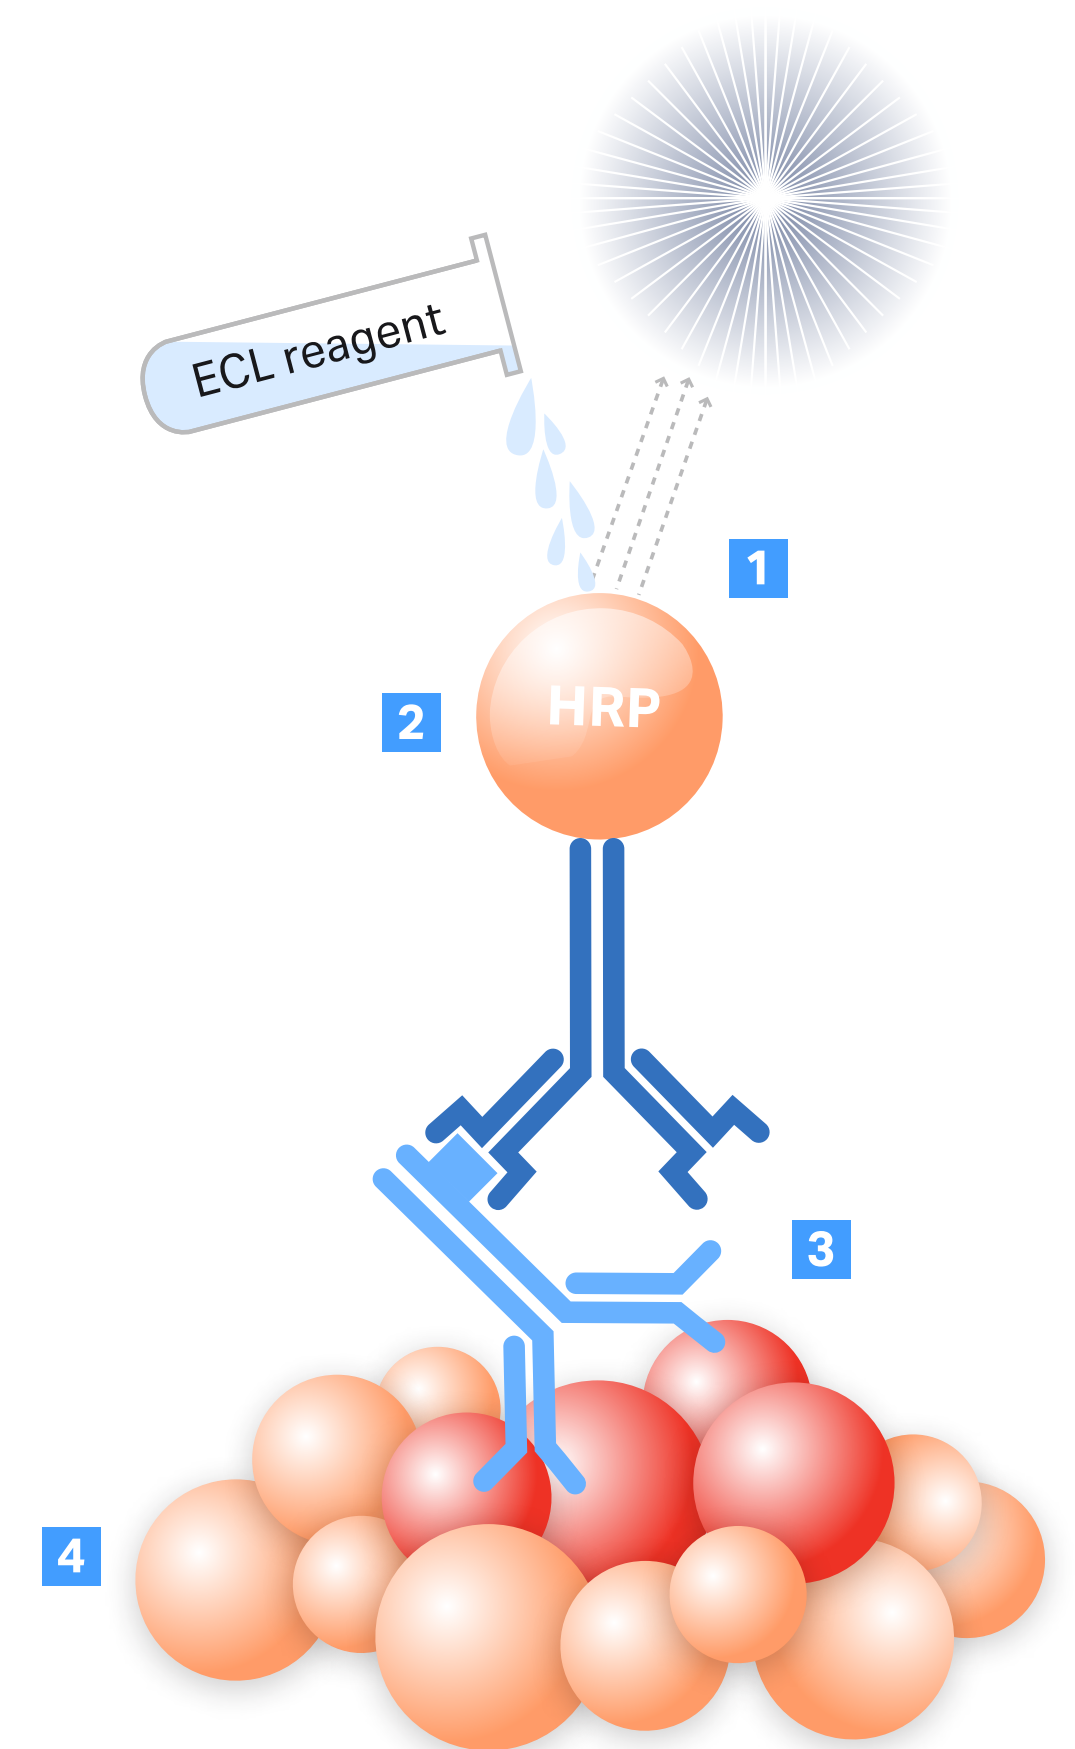


Fig 1. The principle of chemiluminescent Western blotting detection.

Amersham ECL

- One of the first commercially available chemiluminescent detection reagents
- Entry-level chemiluminescent detection reagent
- Reagent of choice for confirmatory Western blotting applications

Western blotting is a valuable tool for verifying identity of recombinantly expressed proteins, as well as for identification of protein fractions to be used for further enrichment of the target molecule (Fig 2).

Amersham ECL Prime

- A highly sensitive chemiluminescent Western blotting detection reagent
- Intense and long lasting signal, enabling large experimental series
- Accurate detection of both high and low abundant proteins on the same blot

Amersham ECL Prime is a highly sensitive detection system characterized by an extremely stable signal emission, allowing for repeated exposures and facilitating processing of several blots in the same experimental run. In addition, the high intensity of the emitted signal makes Amersham ECL Prime suitable for detection of low abundance proteins (Fig 3).

Amersham ECL Select

- The most sensitive chemiluminescent Western blotting detection reagent in the Amersham ECL product range
- Exceptional signal intensity, resulting in bright, clear bands even at low protein levels
- Offers high sensitivity even when using highly diluted primary and secondary antibodies

The high signal intensity makes Amersham ECL Select™ reagent suitable for the most demanding Western blotting applications, including detection of minute protein quantities (Fig 4). The high sensitivity and the broad linear dynamic range of Amersham ECL Select enables qualitative as well as quantitative analyses. Amersham ECL Select reagent generates very intense light emission, allowing for use with highly diluted antibodies in your experiments.

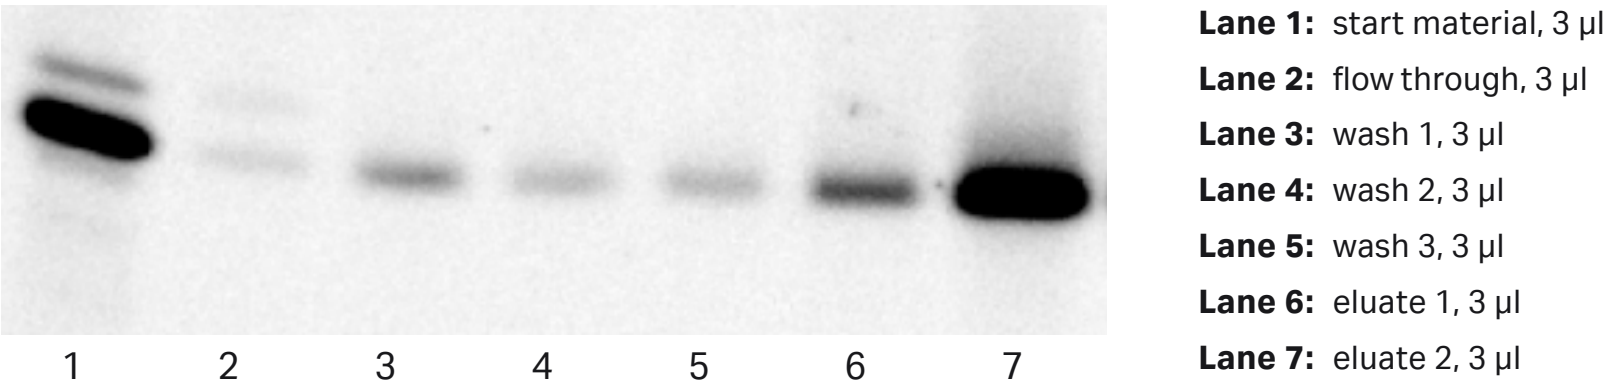


Fig 2. Amersham™ ECL Western blotting detection reagent used for confirmation of histidine-EGFP, recombinantly expressed in Sf21 insect cells and enriched using Mag Sepharose™ magnetic beads.

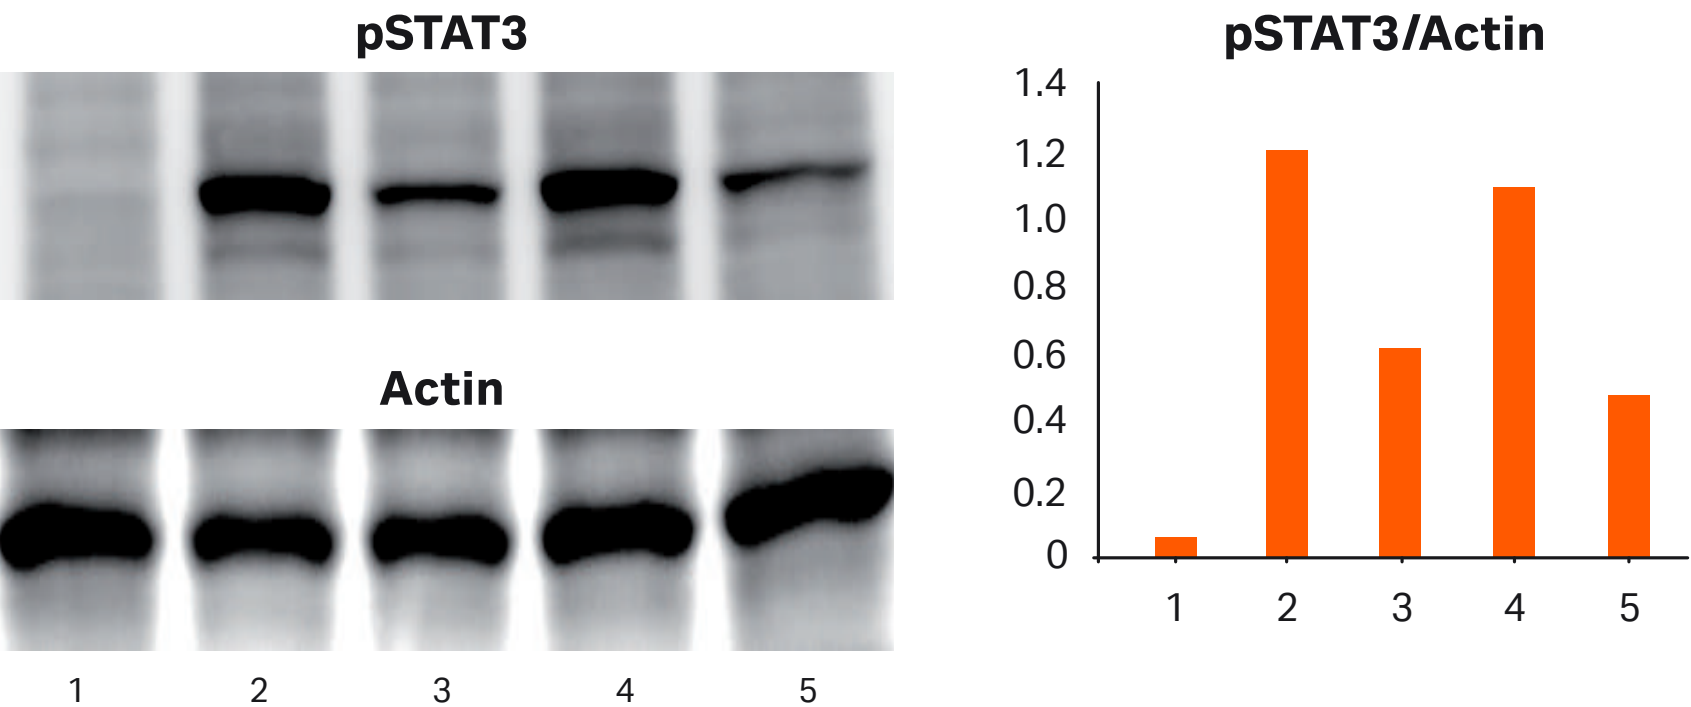


Fig 3. Western blotting detection of Tyr705-phosphorylated STAT3 (pSTAT3) in five different HeLa cell lysates. In each sample, the target protein was quantified relatively to actin levels in the same lysate. The target protein was detected using Amersham ECL Prime.


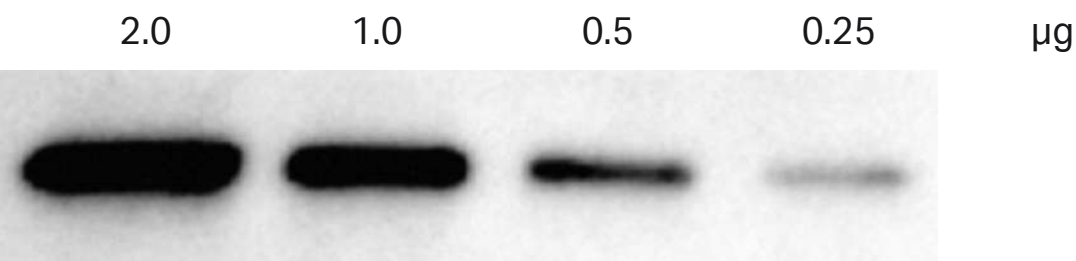


Fig 4. Western blotting detection of endogenous TAB 1 in 293 T cell lysates. The high signal intensity of Amersham ECL Select generates bright bands and offers highly sensitive detection.

Selection guide – Amersham ECL Western blotting detection reagents

Choose a detection reagent depending on the purpose of your experiment

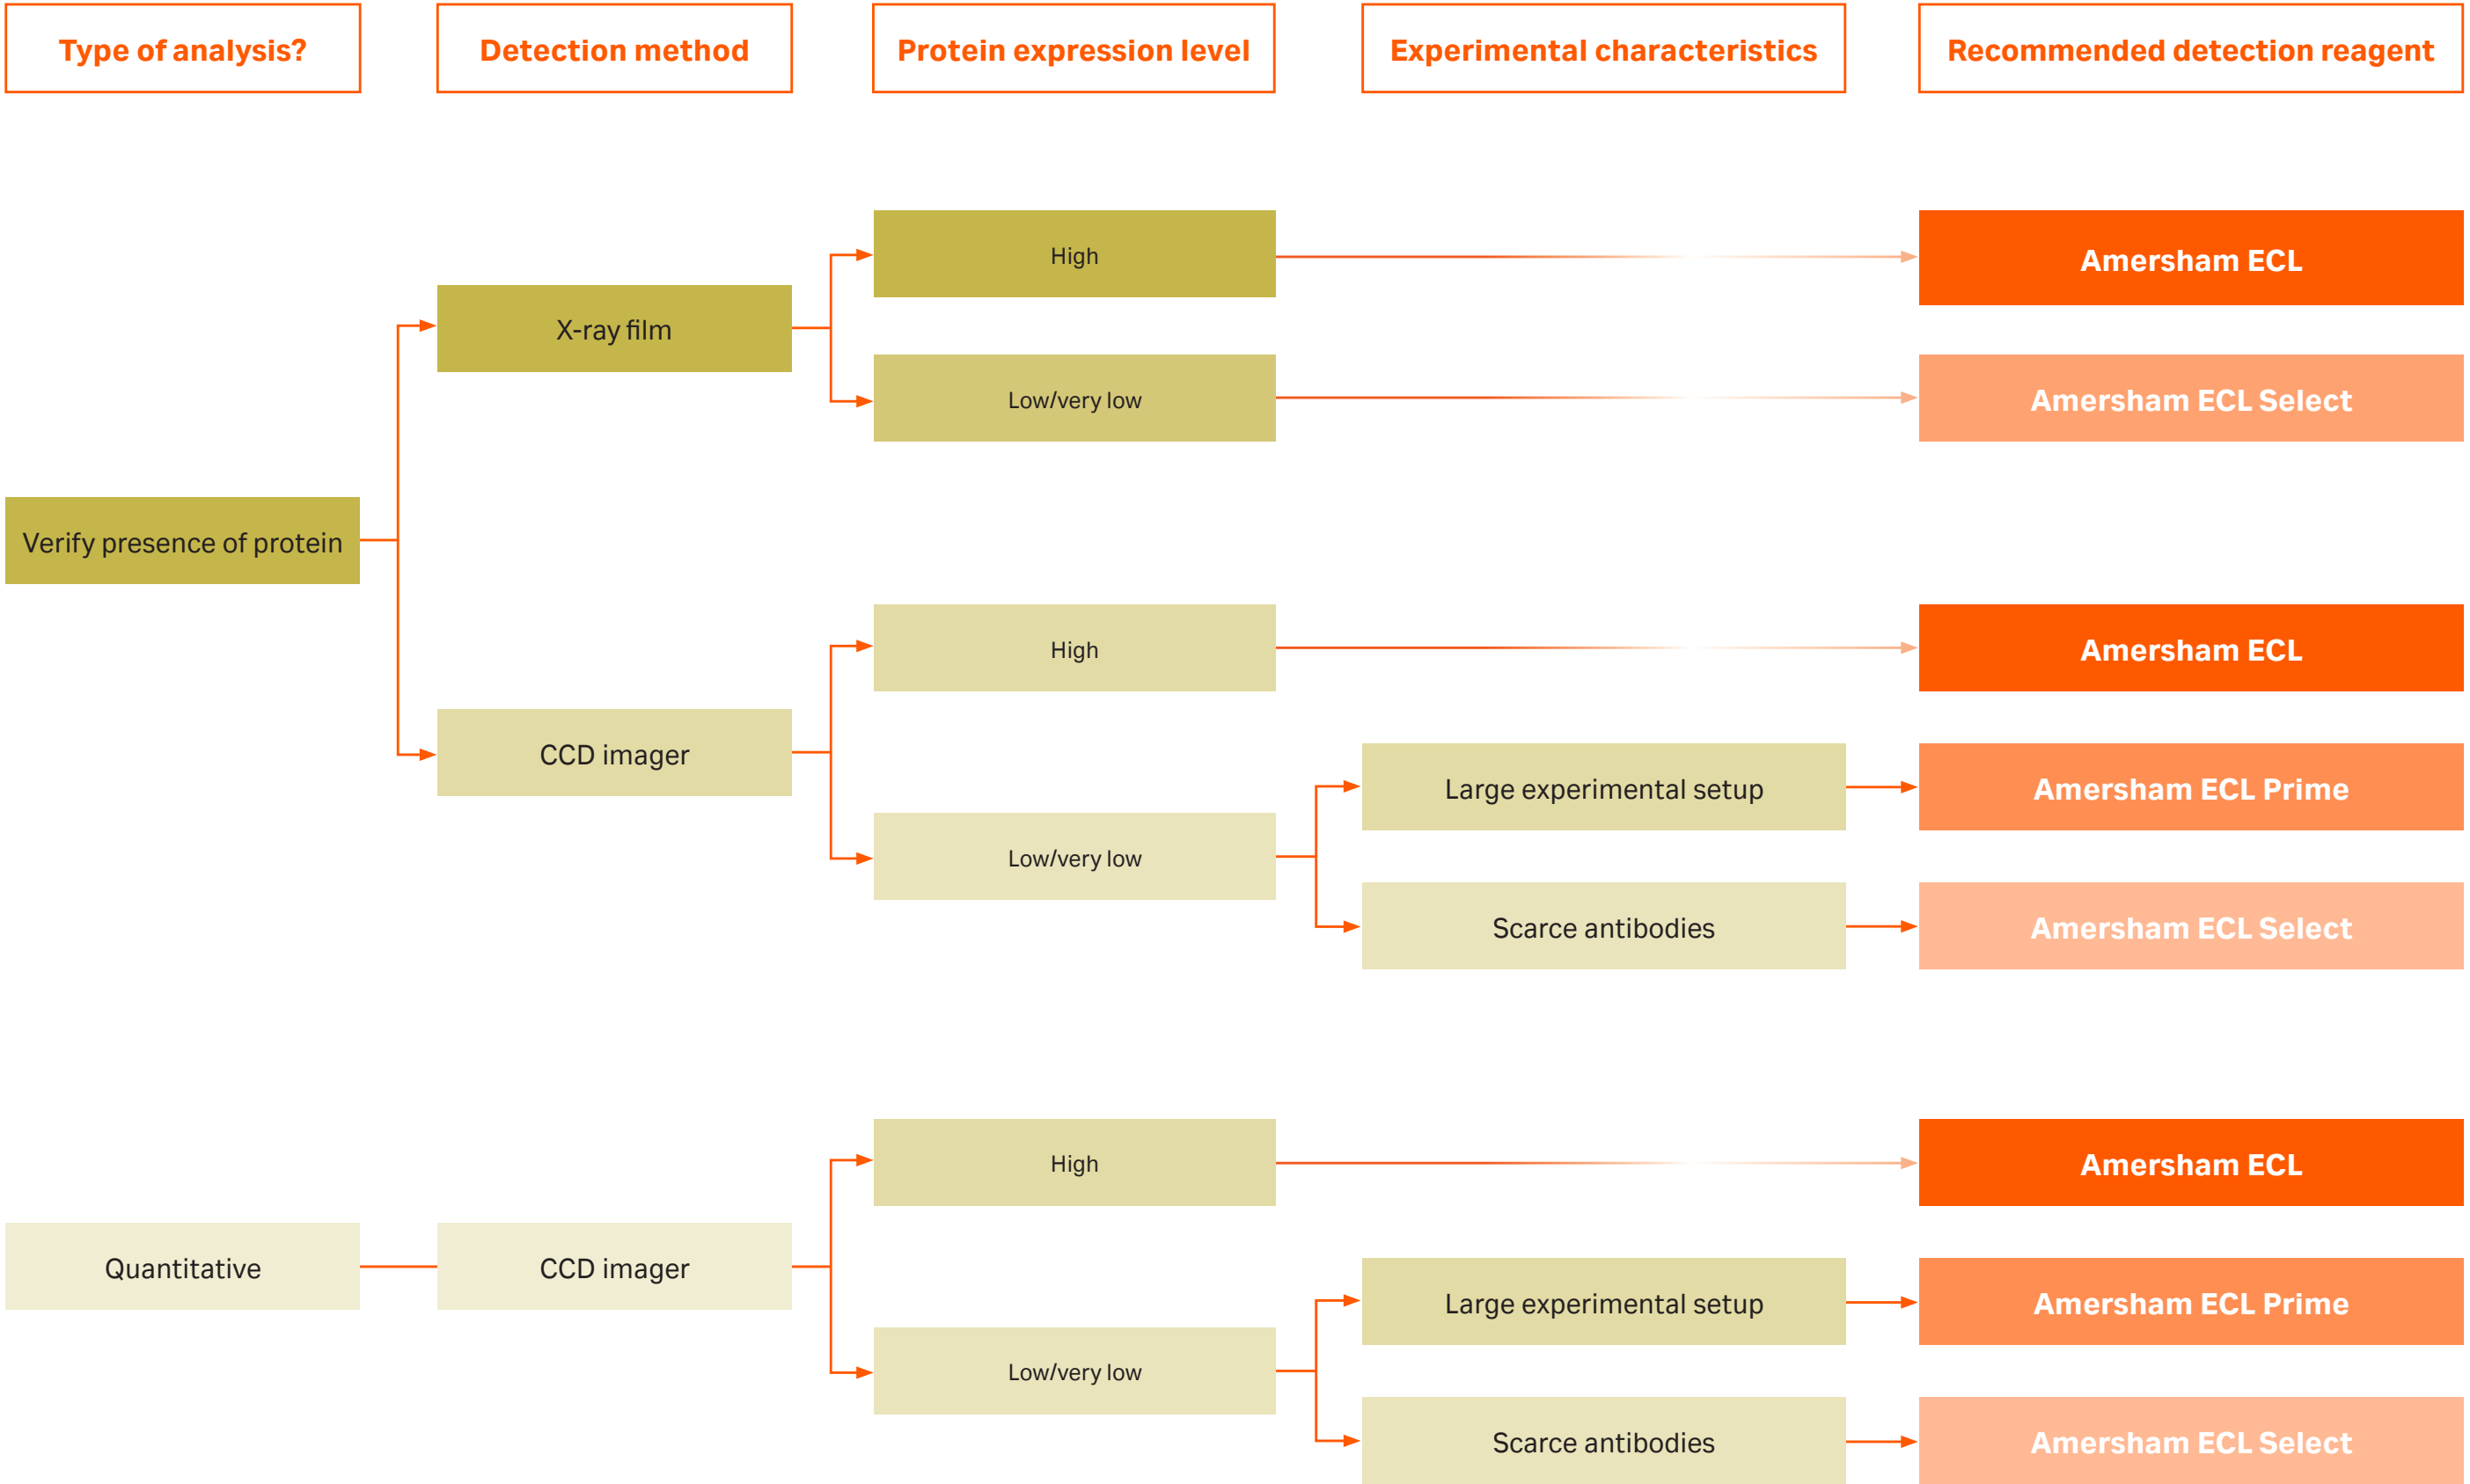

Benchmarking data

Amersham ECL

Figure 5 shows a side-by-side comparison of Amersham ECL reagent with other chemiluminescence detection reagents in the same sensitivity range.

Samples: Two-fold dilution series of HeLa cell lysate starting at 5 µg
Primary antibody dilution: 1:1000
Secondary antibody dilution: 1:10 000
Detection: Amersham Imager 600, 1 min exposure

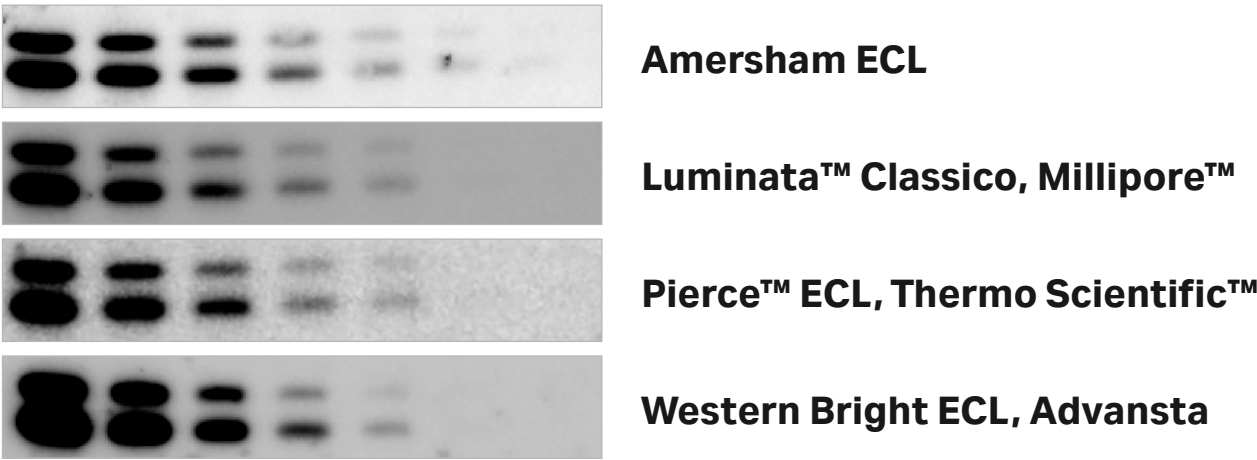


Fig 5. Amersham ECL reagent exhibits similar sensitivity as the competitor reagents in Western blotting detection of ERK 1/2.

Amersham ECL Prime

Figure 6 shows a side-by-side comparison of Amersham ECL Prime with other high-sensitive chemiluminescence detection reagents.

Samples: Two-fold dilution series of HeLa cell lysate starting at 10 µg
Primary antibody dilution: 1:5000
Secondary antibody dilution: 1:30 000
Detection: Amersham Imager 600, 75 s exposure



Fig 6. Amersham ECL Prime exhibits similar sensitivity as the competitor reagents in Western blotting detection of ERK 1/2. The Millipore reagents were slightly less sensitive and also reached saturation at the highest concentrations (10 to 5 µg), decreasing the dynamic range of these reagents.

Figure 7 shows Amersham ECL Prime in comparison with Clarity™ Western ECL Substrate from Bio-Rad.

Samples: Two-fold dilution series of HeLa cell lysate starting at 2.5 µg
Primary antibody dilution: 1:3000
Secondary antibody dilution: 1:30 000
Detection: Amersham Imager 600, 3 min exposure

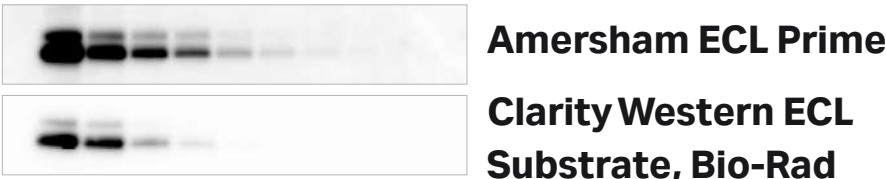


Fig 7. Amersham ECL Prime exhibits higher sensitivity and signal intensity compared with Clarity Western ECL Substrate in Western blotting detection of ERK 1/2.

Amersham ECL Select

Figure 8 shows a side-by-side comparison of Amersham ECL Select with other high-sensitive chemiluminescence detection reagents.

Samples: Two-fold dilution series of HeLa cell lysate starting at 2.5 µg
Primary antibody dilution: 1:10 000
Secondary antibody dilution: 1:100 000
Detection: Amersham Imager 600, 3 min exposure

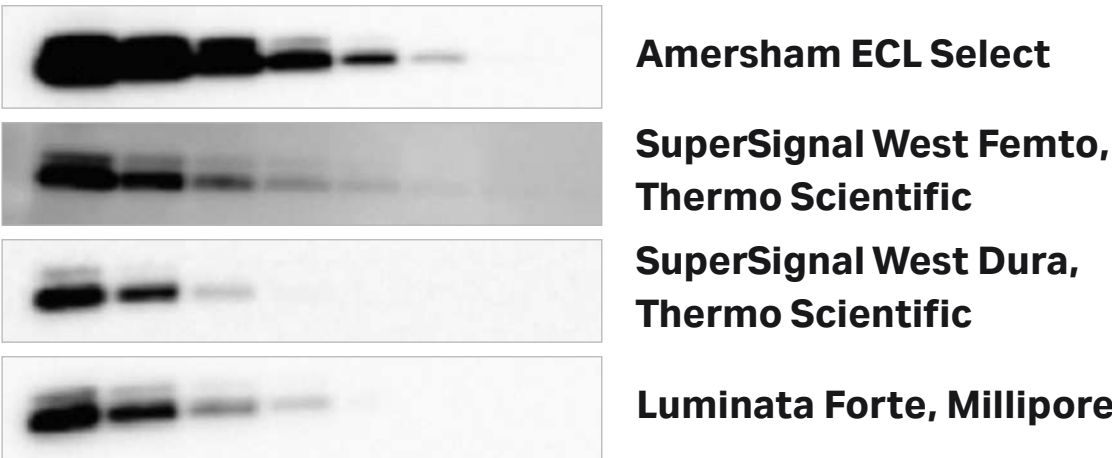


Fig 8. Amersham ECL Select shows brighter bands, lower background, and higher limit of detection compared with competitor reagents in Western blotting detection of ERK 1/2.

Ordering information

Product	Quantity	Code number
Western blotting detection reagents		
Amersham ECL Western Blotting Detection Reagents	For 1000 cm ² membrane	RPN2109
Amersham ECL Western Blotting Detection Reagents	For 2000 cm ² membrane	RPN2209
Amersham ECL Western Blotting Detection Reagents	For 4000 cm ² membrane	RPN2106
Amersham ECL Western Blotting Detection Reagents	For 6000 cm ² membrane	RPN2134
Amersham ECL Prime Western Blotting Detection Reagents	For 1000 cm ² membrane	RPN2232
Amersham ECL Prime Western Blotting Detection Reagents	For 3000 cm ² membrane	RPN2236
Amersham ECL Select Western Blotting Detection Reagents	For 1000 cm ² membrane	RPN2235
Amersham ECL Western Blotting Reagent Pack	For at least 10 miniblots	RPN2124
(Includes detection reagent, secondary antibodies, and blocking agent)		
Western blotting membrane blocking reagent		
Amersham ECL Prime Blocking Reagent	For at least 20 miniblots	RPN418
Amersham ECL Blocking Agent	For at least 20 miniblots	RPN2125
HRP conjugated secondary antibodies		
Amersham ECL HRP Anti-Mouse Secondary antibody	100 µl	NA931-100UL
Amersham ECL HRP Anti-Mouse Secondary antibody	1 ml	NA931-1ML
Amersham ECL HRP Anti-Rabbit Secondary antibody	100 µl	NA934-100UL
Amersham ECL HRP Anti-Rabbit Secondary antibody	1 ml	NA934-1ML
Amersham ECL HRP Anti-Rat Secondary antibody	1 ml	NA935



cytiva.com/amershamwb

Cytiva and the Drop logo are trademarks of Global Life Sciences IP Holdco LLC or an affiliate. Amersham, ECL, ECL Select, and Sepharose are trademarks of Global Life Sciences Solutions USA LLC or an affiliate doing business as Cytiva.

Clarity is a trademark of Bio-Rad Laboratories Inc. Immobilon, Luminata, and Millipore are trademarks of Merck KGaA. Pierce, SuperSignal, and Thermo Scientific are trademarks of Thermo Fisher Scientific.

Amersham ECL Prime or portions thereof is manufactured and sold under license from Cyanagen Srl and is subject of US patent 7,855,287, US Patent 7,803,573, and Italian application number TO2010A000580, together with other equivalent granted patents and patent applications in other countries.

All third party trademarks are the property of their respective owners.

© 2020 Cytiva

All goods and services are sold subject to the terms and conditions of sale of the supplying company operating within the Cytiva business. A copy of those terms and conditions is available on request. Contact your local Cytiva representative for the most current information.

For local office contact information, visit cytiva.com/contact

CY12784-06Nov20-SG

